

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST Daniel McGinnis AGENCY YCSO

DATE 01-13-09 TIME 0412

INTOXILYZER SERIAL # 80-001019 LOCATION Prescott Jail

[Handwritten initials]

1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution .10 AC.
OR

~~Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C~~

[Handwritten initials]

2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.

[Handwritten initials]

4. Air blank completed.
5. Calibration check completed. Test results 0. 098 AC.
6. Air blank completed.
7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Daniel McGinnis 543/8088 QAS# 33426

INTOXILYZER 8000

Location: YCSO PRESCOTT JAIL

Serial Number: 80-001019

01/13/2009

04:12:43

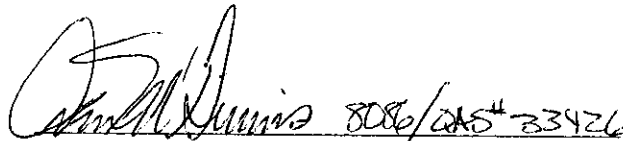
Standard Lot#: 804301I

Last Changed By: D. RAISS #3693

QAS: D. MCGINNIS #8086

YAVAPAI CSO

Test	g/210L	Time
✓ Air Blank	0.000	04:13:10
Cal Check	0.098	04:13:29
Air Blank	0.000	04:13:58


Operator's Signature

8086/QAS# 33426