

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST Daniel McInnis AGENCY YCSO

DATE 01-13-09 TIME 05 56

INTOXILYZER SERIAL # 80-001222 LOCATION Verde Jail

- DM* 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution .10 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. ~~Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C~~
- DM* 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- DM* 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- DM* 4. Air blank completed.
- DM* 5. Calibration check completed. Test results 0. 100 AC.
- DM* 6. Air blank completed.
- DM* 7. Remove printed record. Attach the record to the completed checklist.

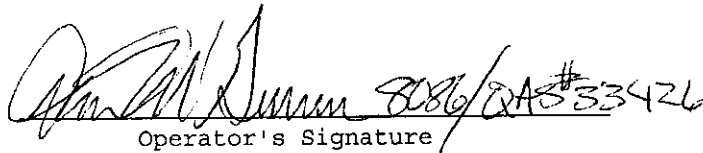
SIGNATURE Daniel McInnis 8086/QAG #33426

INTOXILYZER 8000
Location: YCSO-VERDE JAIL
Serial Number: 80-001222
01/13/2009 05:56:23

Standard Lot#: 804301I
Last Changed By: D. RAISS #3693

QAS: D. MCGINNIS #8086
YAVAPAI CSO

Test	g/210L	Time
Air Blank	0.000	05:56:51
Cal Check	0.100	05:57:09
Air Blank	0.000	05:57:39


Operator's Signature 8086/QAS#33426

INTOXILYZER 8000
Location: YCSO-VERDE JAIL
Serial Number: 80-001222
01/13/2009 05:55:17

Standard Lot#: 804301I
Last Changed By: D. RAISS #3693

QAS: D. MCGINNIS #8086
YAVAPAI CSO

Test	g/210L	Time
Air Blank	AMB*	05:55:45
Air Blank	0.000	05:56:13

*Ambient Fail

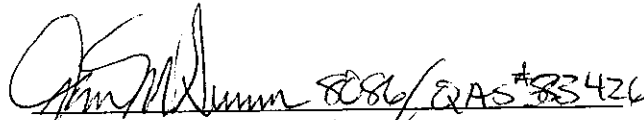

Operator's Signature

EXHIBIT G-4
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Daniel McGinnis AGENCY YLSO

DATE 01-13-09 TIME 0547

INTOXILYZER SERIAL # 80-001222 LOCATION Verde Jail

DM 1. Display Reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS
DM 1. Clock time check.
DM 2. Date check.

OPERATIONAL TESTS
DM 1. Alcohol-free subject test result 0. 000 AC.
DM 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
DM 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.

DM 4. Standard Calibration Check standard 0. 10 AC. Result 0. 102 AC.

Instrument is operating properly and accurately. YES DM NO _____

COMMENTS Ambient Fail w/ second Cal. Check

SIGNATURE Daniel McGinnis 8086 / QAS #33426

INTOXILYZER 8000
Location: YCSO-VERDE JAIL
Serial Number : 80-001222
01/13/2009 05:42:19

Standard Lot#: 804301I
Last Changed By: D. RAISS #3693

QAS: D. MCGINNIS #8086
YAVAPAI CSO

Operator: D. MCGINNIS #8086
YAVAPAI CSO

Subject: SQAP,TEST
DOB: 09/09/1963
Sex: M Weight: 220

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	05:43:33
Diagnostic Test	Pass	05:44:01
Air Blank	0.000	05:44:28
0.100 Cal Check	0.101	05:44:47
Air Blank	0.000	05:45:17
Subject Test	0.000	05:46:01
Air Blank	ABT*	05:46:11
Air Blank	RFI**	05:46:18

*Sequence Aborted

**RFI Detect

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: YCSO-VERDE JAIL
Serial Number : 80-001222
01/13/2009

05:47:02

Standard Lot#: 804301I
Last Changed By: D. RAISS #3693

QAS: D. MCGINNIS #8086
YAVAPAI CSO

Operator: D. MCGINNIS #8086
YAVAPAI CSO

Subject: SQAP,TEST
DOB: 09/09/1963
Sex: M Weight: 220

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	05:48:02
Diagnostic Test	Pass	05:48:30
Air Blank	0.000	05:48:57
0.100 Cal Check	0.102	05:49:16
Air Blank	0.000	05:49:46
Subject Test	0.090*	05:52:54
Air Blank	0.000	05:53:26
Air Blank	0.000	05:53:54
Subject Test	XXX**	05:54:30
Air Blank	IPS***	05:54:38

*Deficient Sample

**Invalid Sample

Begin new deprivation period

***Improper Sample

Not a Successfully Completed Test Sequence

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST David McGinnis AGENCY YCSO
DATE 01-13-09 TIME 0539
INTOXILYZER SERIAL # 80-001222 LOCATION Verde Jail

- 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution .10 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- 4. Air blank completed.
- 5. Calibration check completed. Test results 0. 101 AC.
- 6. Air blank completed.
- 7. Remove printed record. Attach the record to the completed checklist.

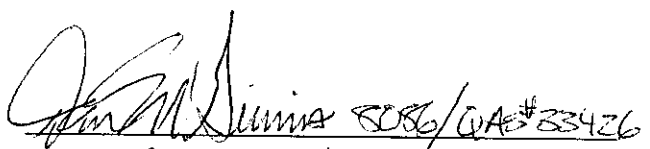
SIGNATURE David McGinnis 8086/QAS# 33426

INTOXILYZER 8000
Location: YCSO-VERDE JAIL
Serial Number: 80-001222
01/13/2009 05:39:26

Standard Lot#: 804301I
Last Changed By: D. RAISS #3693

QAS: D. MCGINNIS #8086
YAVAPAI CSO

Test	g/210L	Time
Air Blank	0.000	05:39:53
Cal Check	0.101	05:40:12
Air Blank	0.000	05:40:41


Operator's Signature