

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST Daniel McInnis AGENCY VCSO

DATE 05-05-09 TIME 2207

INTOXILYZER SERIAL # 80-001222 LOCATION Verde Jail

- [Signature]* 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 10 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- [Signature]* 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- [Signature]* 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- [Signature]* 4. Air blank completed.
- [Signature]* 5. Calibration check completed. Test results 0. 103 AC.
- [Signature]* 6. Air blank completed.
- [Signature]* 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE

[Signature] 543/OAS #33426

INTOXILYZER 8000
Location: YCSO-VERDE JAIL
Serial Number: 80-001222
05/05/2009 22:07:17

Standard Lot#: 901401I
Last Changed By: D. MCGINNIS #8086

QAS: D. MCGINNIS #8086
YAVAPAI CSO

Test	g/210L	Time
Air Blank	0.000	22:07:45
Cal Check	0.103	22:08:04
Air Blank	0.000	22:08:33

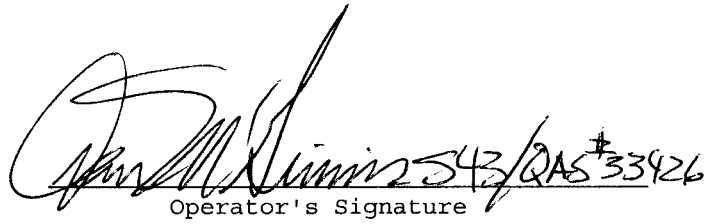

Operator's Signature

EXHIBIT G-4
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Daniel McGinnis AGENCY YCSO

DATE 05-05-09 TIME 2209

INTOXILYZER SERIAL # 80-001222 LOCATION Verde Jail

DM Display Reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- DM 1. Clock time check.
DM 2. Date check.

OPERATIONAL TESTS

- DM 1. Alcohol-free subject test result 0. 00 AC.
DM 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
DM 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
DM 4. Standard Calibration Check standard 0. 10 AC. Result 0. 107 AC.

Instrument is operating properly and accurately. YES DM NO _____

COMMENTS

All OK
changed Gas Standard bottle Lot #90140/I EXP 01/23/2011

SIGNATURE Daniel McGinnis S43/QAS # 33426

INTOXILYZER 8000
Location: YCSO-VERDE JAIL
Serial Number : 80-001222
05/05/2009

22:14:20

Standard Lot#: 901401I
Last Changed By: D. MCGINNIS #8086

QAS: D. MCGINNIS #8086
YAVAPAI CSO

Operator: D. MCGINNIS #8086
YAVAPAI CSO

Subject: SQAP,TEST
DOB: 09/09/1990
Sex: M Weight: 200

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	22:15:18
Diagnostic Test	Pass	22:15:45
Air Blank	0.000	22:16:13
0.100 Cal Check	0.100	22:16:31
Air Blank	0.000	22:17:01
Subject Test	0.084*	22:20:09
Air Blank	0.000	22:20:42
Air Blank	0.000	22:21:09
Subject Test	XXX**	22:21:36
Air Blank	IPS***	22:21:44

*Deficient Sample

**Invalid Sample

Begin new deprivation period

***Improper Sample

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: YCSO-VERDE JAIL
Serial Number : 80-001222
05/05/2009

22:09:48

Standard Lot#: 901401I
Last Changed By: D. MCGINNIS #8086

QAS: D. MCGINNIS #8086
YAVAPAI CSO

Operator: D. MCGINNIS #8086
YAVAPAI CSO

Subject: SQAP,TEST
DOB: 09/09/1990
Sex: M Weight: 200

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	22:10:41
Diagnostic Test	Pass	22:11:08
Air Blank	0.000	22:11:35
0.100 Cal Check	0.101	22:11:54
Air Blank	0.000	22:12:24
Subject Test	0.000	22:13:04
Air Blank	0.000	22:13:31
Five Minute Wait	ABT*	
Air Blank	RFI**	22:13:47

*Sequence Aborted

**RFI Detect

Not a Successfully Completed Test Sequence

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST Daniel McGinnis AGENCY YCSO

DATE 05-05-09 TIME 2224

INTOXILYZER SERIAL # 80-001222 LOCATION Verde Jail

- [Signature]* 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution .10 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach ~~34°C ± 0.2°C~~
- [Signature]* 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- [Signature]* 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- [Signature]* 4. Air blank completed.
- [Signature]* 5. Calibration check completed. Test results 0. 101 AC.
- [Signature]* 6. Air blank completed.
- [Signature]* 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Daniel McGinnis 543/QAS #33426

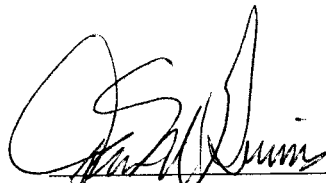
INTOXILYZER 8000
Location: YCSO-VERDE JAIL
Serial Number: 80-001222
05/05/2009

22:24:15

Standard Lot#: 901401I
Last Changed By: D. MCGINNIS #8086

QAS: D. MCGINNIS #8086
YAVAPAI CSO

Test	g/210L	Time
Air Blank	0.000	22:24:42
Cal Check	0.101	22:25:01
Air Blank	0.000	22:25:31


D. McGinnis 543/QAS #33426
Operator's Signature

INTOXILYZER 8000

Location: YCSO-VERDE JAIL

Serial Number: 80-001222

05/05/2009

22:22:30

Standard Lot#: 901401I

Last Changed By: D. MCGINNIS #8086

QAS: D. MCGINNIS #8086

YAVAPAI CSO

Test	g/210L	Time
Air Blank	AMB*	22:22:58
Air Blank	0.000	22:23:26

*Ambient Fail


Operator's Signature