

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)
ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST Daniel McGinnis AGENCY YLSO
DATE 07-01-09 TIME 2228
INTOXILYZER SERIAL # 80-001222 LOCATION Verde Jail

DM
DM
DM
DM
DM

1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0.10 AC.
~~Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$~~
2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
4. Air blank completed.
5. Calibration check completed. Test results 0. 099 AC.
6. Air blank completed.
7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE *Daniel McGinnis* S43/QAS #33426

INTOXILYZER 8000
Location: YCSO-VERDE JAIL
Serial Number: 80-001222
07/01/2009

22:28:25

Standard Lot#: 901401I
Last Changed By: D. MCGINNIS #8086

QAS: D. MCGINNIS #8086
• YAVAPAI CSO

Test	g/210L	Time
Air Blank	0.000	22:28:53
Cal Check	0.099	22:29:11
Air Blank	0.000	22:29:41

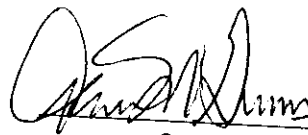

Operator's Signature 543/QAS #33126

EXHIBIT G-4
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST Daniel McGinnis AGENCY YCSO

DATE 07-01-09 TIME 2230

INTOXILYZER SERIAL # 80-001222 LOCATION Verde Jail

DM 1. Display Reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- 1. Clock time check.
- 2. Date check.

OPERATIONAL TESTS

DM 1. Alcohol-free subject test result 0. 000 AC.

DM 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed

DM 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.

DM 4. Standard Calibration Check standard 0. 100 AC. Result 0. 098 AC.

Instrument is operating properly and accurately. YES DM NO DM

COMMENTS All OK

SIGNATURE Daniel McGinnis 543/QAS # 33426

INTOXILYZER 8000
Location: YCSO-VERDE JAIL
Serial Number : 80-001222
07/01/2009

22:30:54

Standard Lot#: 901401I
Last Changed By: D. MCGINNIS #8086

QAS: D. MCGINNIS #8086
YAVAPAI CSO

Operator: D. MCGINNIS #8086
YAVAPAI CSO

Subject: SQAP, TEST
DOB: 09/09/1990
Sex: M Weight: 200

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	22:31:52
Diagnostic Test	Pass	22:32:19
Air Blank	0.000	22:32:47
0.100 Cal Check	0.100	22:33:05
Air Blank	0.000	22:33:35
Subject Test	0.000	22:34:08
Air Blank	ABT*	22:34:16
Air Blank	RFI**	22:34:26

*Sequence Aborted

**RFI Detect

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location: YCSO-VERDE JAIL

Serial Number : 80-001222

07/01/2009

22:34:39

Standard Lot#: 901401I

Last Changed By: D. MCGINNIS #8086

QAS: D. MCGINNIS #8086

YAVAPAI CSO

Operator: D. MCGINNIS #8086

YAVAPAI CSO

Subject: SQAP,TEST

DOB: 09/09/1990

Sex: M Weight: 200

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	22:35:43
Diagnostic Test	Pass	22:36:11
Air Blank	0.000	22:36:38
0.100 Cal Check	0.099	22:36:57
Air Blank	0.000	22:37:27
Subject Test	0.072*	22:40:35
Air Blank	0.000	22:41:07
Air Blank	0.000	22:41:34
Subject Test	XXX**	22:42:00
Air Blank	IPS***	22:42:08

*Deficient Sample

**Invalid Sample

Begin new deprivation period

***Improper Sample

Not a Successfully Completed Test Sequence

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST Daniel McGinnis AGENCY YCSO

DATE 07-01-09 TIME 2243

INTOXILYZER SERIAL # 80001222 LOCATION Verde Jail

DM

1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution .10 AC.
OR

~~Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C~~

DM

2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"

3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.

DM

4. Air blank completed.

DM

5. Calibration check completed. Test results 0. 0.08 AC.

DM

6. Air blank completed.

7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE *Daniel McGinnis* SHB/QAS# 33426

INTOXILYZER 8000
Location: YCSO-VERDE JAIL
Serial Number: 80-001222
07/01/2009

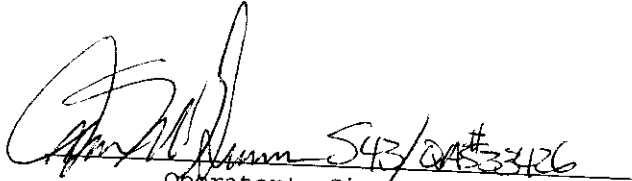
22:42:56

Standard Lot#: 901401I
Last Changed By: D. MCGINNIS #8086

QAS: D. MCGINNIS #8086
YAVAPAI CSO

Test	g/210L	Time
Air Blank	AMB*	22:43:24
Air Blank	0.000	22:43:52

*Ambient Fail


Operator's Signature

INTOXILYZER 8000

Location: YCSO-VERDE JAIL

Serial Number: 80-001222

07/01/2009

22:43:59

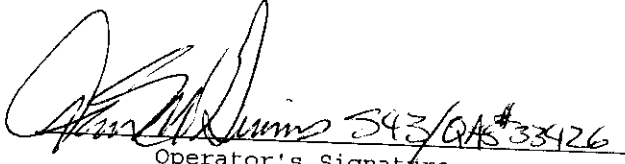
Standard Lot#: 901401I

Last Changed By: D. MCGINNIS #8086

QAS: D. MCGINNIS #8086

YAVAPAI CSO

Test	g/210L	Time
Air Blank	0.000	22:44:27
Cal Check	0.098	22:44:45
Air Blank	0.000	22:45:15


Operator's Signature