

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST D. Ashby #562 AGENCY YCSO

DATE 3-25-09 TIME 0623

INTOXILYZER SERIAL # 80-001455 LOCATION Bagdad Substation

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 100 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Deann Ashby #562 / OAS #33400

INSTRUMENT# 3000

Location: YAVAPAI CO, FLAGSTAD

Serial Number: 60-001455

03/25/2009

06/24/11

Standard Lot#: 7309011

Last Changed By: D. ASHBY #562

QAS: D. ASHBY #562

YAVAPAI CO

Test	g/210L	Time
Air Blank	0.000	06/24/11
Cal Check	0.100	06/24/11
Air Blank	0.000	06/24/11

Deann J. Ashby #562/QAS#33400
Operator's Signature

EXHIBIT G-4
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST D. Ashby #562 AGENCY YCSO

DATE 3.25.09 TIME 0630

INTOXILYZER SERIAL # 80-001455 LOCATION Bagdad Substation

(✓) 1. Display Reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

(✓) 1. Clock time check.

(✓) 2. Date check.

OPERATIONAL TESTS

(✓) 1. Alcohol-free subject test result 0. 000 AC.

(✓) 2. Error recognition logic system functioning.

Not a Successfully Completed Test Sequence printed

(✓) 3. Proper sample recognition system.

Not a Successfully Completed Test Sequence printed

Deficient sample printed.

(✓) 4. Standard Calibration Check standard 0. 100 AC. Result 0. 100 AC.

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE Deann J Ashby #562 / QAS# 33400

INTOXILYZER 8000

Location: YAVAPAI SO, BAGDAD

Serial Number : 80-001455

03/25/2009

06:27:00

Standard Lot#: 7309011

Last Changed By: D. ASHBY

06:27:00

QAS: D. ASHBY

06:27:00

YAVAPAI CSO

Operator: D. ASHBY

06:27:00

YAVAPAI CSO

Subject: SOAP, TEST

DOB: 01/01/1999

Sex: M

Weight: 150

15 Minute Deprivation Period: Yes

Test	g/210L	Time
Air Blank	0.000	06:27:00
Diagnostic Test	Pass	06:28:00
Air Blank	0.000	06:29:00
0.100 Cal Check	0.100	06:30:00
Air Blank	0.000	06:31:00
Subject Test	0.000	06:32:00
Air Blank	0.000	06:33:00
Five Minute Wait	ABT*	
Air Blank	0.000	06:34:00

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location: YAVAPAI CO. BACHELOR

Serial Number : 80-001455

03/25/2009

00:31:19

Standard Lot#: 7309010

Last Changed By: D. ASHBY

3/25/09

OAS: D. ASHBY

3/25/09

YAVAPAI CSO

Operator: D. ASHBY

3/25/09

YAVAPAI CSO

Subject: SQAP, TEST

DOB: 01/01/1999

Sex: M

Weight: 150

15 Minute Deprivation Period: Yes

Test	g/210L	Time
Air Blank	URS*	00:31:19
Air Blank	0.000	00:32:14

*Improper Sample

Not a Successfully Completed Test Report

INTOXILYZER 8000

Location: YAVAPAI CO, BACEND

Serial Number : 88-001155

03/25/2009

06:12:12

Standard Lot#: 7309013

Last Changed By: D. ASHBY

12:57

OAS: D. ASHBY

12:58

YAVAPAI CSO

Operator: D. ASHBY

12:59

YAVAPAI CSO

Subject: SOAP,TEST

DOB: 01/01/1999

Sex: M

Weight: 150

15 Minute Deprivation Period? 200

Test	g/210L	Time
Air Blank	REFL	06:13:11
Air Blank	0.000	06:13:12

*REFL Detect

Not a Successfully Completed Test Sequence

INFORMATION 8000

Location: YAVAPAI CO, RMT 03

Serial Number : 96-001155

03/25/2009

96-001155

Standard Lot#: 7309011

Last Changed By: D. ASHBY

1998

QAS: D. ASHBY

YAVAPAI CO

Operator: D. ASHBY

19

YAVAPAI CO

Subject: COAL, TEST

DOB: 01/01/1969

Sex: M

Weight: 50

15 Minute Deprivation Period

Test	g/210L	Time
Air Blank	0.000	03/25/09
Diagnostic Test	Pass	03/25/09
Air Blank	0.000	03/25/09
0.100 Cal Check	0.100	03/25/09
Air Blank	0.000	03/25/09
Subject Test	0.0627	03/25/09
Air Blank	0.000	03/25/09
Air Blank	0.000	03/25/09
Subject Test	0.0627	03/25/09
Air Blank	0.000	03/25/09

*Deficient Sample

*Invalid Sample

Begin new deprivation period

Not a successfully completed test

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST D. Ashby #562 AGENCY YCSO

DATE 3-25-09 TIME 0645

INTOXILYZER SERIAL # 80-145 001455 LOCATION Bagdad Substation

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 100 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Diana Ashby #562 / GAS # 33400

INTOXLYZER 3000

Location: YAVAPAI CO, BAGUAD

Serial Number: 09-201355

03/25/2009

00-0000

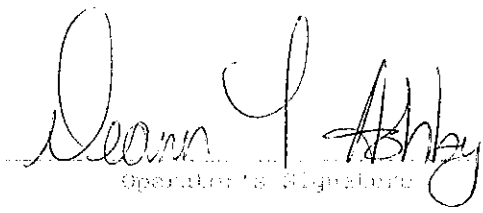
Standard Lot#: 7109011

Last Changed By: D. ASHBY #362

QAS: D. ASHBY #362

YAVAPAI CO

Test	g/200ul	g/l
Air Blank	0.000	0.00000
Cal Check	0.100	0.00100
All Blank	0.000	0.00000

 #562 / QAS # 33400
Operator's Signature