

EXHIBIT G-4
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST D. Ashby #562/QAS#33400 AGENCY YCSO

DATE 11-26-08 TIME 0945

INTOXILYZER SERIAL # 80-001456 LOCATION Yarnell Substation

() 1. Display Reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

() 1. Clock time check.

() 2. Date check.

OPERATIONAL TESTS

() 1. Alcohol-free subject test result 0. 000 AC.

() 2. Error recognition logic system functioning.

Not a Successfully Completed Test Sequence printed

() 3. Proper sample recognition system.

Not a Successfully Completed Test Sequence printed

Deficient sample printed.

() 4. Standard Calibration Check standard 0. 100 AC. Result 0. 098 AC.

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE D. Ashby #562/QAS#33400

INTOXILYZER 8000

Location: YAVAPAI SO YARNELL

Serial Number : 80-001456

11/26/2008

09:38:54

Standard Lot#: 730901I

Last Changed By: C. KROGEDAL

#6535

QAS: D. ASHBY

#S62

YAVAPAI CSO

Operator: D. ASHBY

#S62

YAVAPAI CSO

Subject: SQAP, TEST

DOB: 01/01/1999

Sex: M

Weight: 150

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	09:39:54
Diagnostic Test	Pass	09:40:22
Air Blank	0.000	09:40:49
0.100 Cal Check	0.098	09:41:08
Air Blank	0.000	09:41:37
Subject Test	0.000	09:41:56
Air Blank	0.000	09:42:23
Five Minute Wait	ABT*	
Air Blank	0.000	09:42:59

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: YAVAPAI SO YARNELL
Serial Number : 80-001456
11/26/2008

09:43:46

Standard Lot#: 730901I
Last Changed By: C. KROGEDAL #6535

QAS: D. ASHBY #S62
YAVAPAI CSO

Operator: D. ASHBY #S62
YAVAPAI CSO

Subject: SQAP,TEST

DOB: 01/01/1999

Sex: M Weight: 150

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	IPS*	09:44:32
Air Blank	0.000	09:45:00

*Improper Sample

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location: YAVAPAI SO YARNELL

Serial Number : 80-001456

11/26/2008

09:45:09

Standard Lot#: 730901I

Last Changed By: C. KROGEDAL

#6535

QAS: D. ASHBY

#S62

YAVAPAI CSO

Operator: D. ASHBY

#S62

YAVAPAI CSO

Subject: SQAP, TEST

DOB: 01/01/1999

Sex: M

Weight: 150

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	RFI*	09:45:40
Air Blank	0.000	09:46:09

*RFI Detect

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location: YAVAPAI SO YARNELL

Serial Number : 80-001456

11/26/2008

09:46:17

Standard Lot#: 730901I

Last Changed By: C. KROGEDAL #6535

QAS: D. ASHBY #S62

YAVAPAI CSO

Operator: D. ASHBY #S62

YAVAPAI CSO

Subject: SQAP,TEST

DOB: 01/01/1999

Sex: M

Weight: 150

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	09:47:05
Diagnostic Test	Pass	09:47:32
Air Blank	0.000	09:48:00
0.100 Cal Check	0.098	09:48:18
Air Blank	0.000	09:48:48
Subject Test	0.029*	09:51:56
Air Blank	0.000	09:52:28
Air Blank	0.000	09:52:56
Subject Test	XXX**	09:53:47
Air Blank	0.000	09:54:22

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST D. Ashby #562/QAS#3340 AGENCY YCSO

DATE 11-26-08 TIME 0958

INTOXILYZER SERIAL # 80-001456 LOCATION Yarnell Substation

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 098 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Deann J Ashby #562/QAS#3340

INTOXILYZER 8000

Location: YAVAPAI SO YARNELL

Serial Number: 80-001456

11/26/2008

09:55:34

Standard Lot#: 730901I

Last Changed By: C. KROGEDAL #6535

QAS: D. ASHBY #S62

YAVAPAI CSO

Test g/210L Time

Air Blank 0.000 09:56:01
Cal Check 0.098 09:56:20
Air Blank 0.000 09:56:50

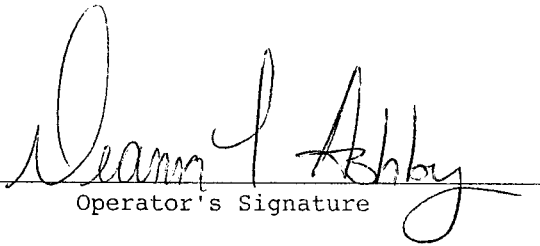

Operator's Signature

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST D. Ashby #812 ^{#QAS 33400} AGENCY YCSO
DATE 11-26-08 TIME 09
INTOXILYZER SERIAL # 80-001456 LOCATION Yarnell Substation

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 0.100 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 0.98 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Deanna Y Ashby #812 / QAS # 33400

INTOXILYZER 8000

Location: YAVAPAI SO YARNELL

Serial Number: 80-001456

11/26/2008

09:36:57

Standard Lot#: 7309011

Last Changed By: C. KROGEDAL #6535

QAS: D. ASHBY #S62

YAVAPAI CSO

Test	g/210L	Time
Air Blank	0.000	09:37:24
Cal Check	0.098	09:37:43
Air Blank	0.000	09:38:13

Dawn I Ashby #S62/QAS #33400

Operator's Signature