

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY

STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST D Ashby #562 AGENCY Y080

DATE 12-24-08 TIME 0734

INTOXILYZER SERIAL # 80-11456 LOCATION YARNELL SUBSTATION

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 4.00 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0.098 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE Dawn J Ashby #562 DAS # 33400

DPS Form Exh G-2 (Rev 05-01)

INTOXILYZER 8000
Location: YUJAPAI CSO YARNELL
Serial Number: 50-011456
12/24/2008 07:34:34

Standard Lot#: 7309011
Last Changed By: C. KROEDER #6535

OAS: C. ASHBY #562
YUJAPAI CSO

Test	Result	Time
Air Blank	0.000	07:35:02
Cal Check	0.098	07:35:20
Air Blank	0.000	07:35:50

Dawn J Ashby
Operator's Signature

EXHIBIT G-4
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000
STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST D. Ashby #562 AGENCY NC80
DATE 12-24-08 TIME 0739
INTOXILYZER SERIAL # 80-00456 LOCATION Yarpe

() 1. Display Reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

- () 1. Clock time check.
() 2. Date check.

OPERATIONAL TESTS

- () 1. Alcohol-free subject test result 0. 000 AC.
() 2. Error recognition logic system functioning.
Not a Successfully Completed Test Sequence printed
() 3. Proper sample recognition system.
Not a Successfully Completed Test Sequence printed
Deficient sample printed.
() 4. Standard Calibration Check standard 0. 1000 AC. Result 0. 007 AC.

Instrument is operating properly and accurately. YES NO

COMMENTS

SIGNATURE D. Ashby #562 GAS# 33400

INTOXILYZER 8000

Location: YAVAPAI SO YARNELL

Serial Number : 80-001456

12/24/2008

07:39:53

Standard Lot#: 730901I

Last Changed By: C. KROGEDAL

#6535

QAS: D. ASHBY

#S62

YAVAPAI CSO

Operator: D. ASHBY

#S62

YAVAPAI CSO

Subject: SQAP,TEST

DOB: 01/01/1999

Sex: M

Weight: 150

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	07:41:01
Diagnostic Test	Pass	07:41:28
Air Blank	0.000	07:41:55
0.100 Cal Check	0.098	07:42:14
Air Blank	0.000	07:42:44
Subject Test	0.000	07:43:06
Air Blank	ABT*	07:43:29
Air Blank	0.000	07:43:57

*Sequence Aborted

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: YAVAPAI SO YARNELL
Serial Number : 80-001456
12/24/2008

07:44:27

Standard Lot#: 730901I
Last Changed By: C. KROGEDAL #6535

QAS: D. ASHBY #S62
YAVAPAI CSO

Operator: D. ASHBY #S62
YAVAPAI CSO

Subject: SQAP,TEST

DOB: 01/01/1999

Sex: M Weight: 150

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	IPS*	07:45:30
Air Blank	0.000	07:45:59

*Improper Sample

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location: YAVAPAI SO YARNELL

Serial Number : 80-001456

12/24/2008

07:46:28

Standard Lot#: 730901I

Last Changed By: C. KROGEDAL

#6535

QAS: D. ASHBY

#S62

YAVAPAI CSO

Operator: D. ASHBY

#S62

YAVAPAI CSO

Subject: SQAP,TEST

DOB: 01/01/1999

Sex: M

Weight: 150

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	RFI*	07:46:59
Air Blank	0.000	07:47:27

*RFI Detect

Not a Successfully Completed Test Sequence

INTOXILYZER 8000
Location: YAVAPAI SO YARNELL
Serial Number : 80-001456
12/24/2008

07:47:33

Standard Lot#: 730901I
Last Changed By: C. KROGEDAL #6535

QAS: D. ASHBY #S62
YAVAPAI CSO

Operator: D. ASHBY #S62
YAVAPAI CSO

Subject: SQAP,TEST

DOB: 01/01/1999

Sex: M Weight: 150

15 Minute Deprivation Period? Yes

Test	g/210L	Time
Air Blank	0.000	07:48:22
Diagnostic Test	Pass	07:48:50
Air Blank	0.000	07:49:17
0.100 Cal Check	0.098	07:49:36
Air Blank	0.000	07:50:06
Subject Test	0.066*	07:53:14
Air Blank	0.000	07:53:48
Air Blank	0.000	07:54:16
Subject Test	XXX**	07:54:37
Air Blank	0.000	07:55:12

*Deficient Sample

**Invalid Sample

Begin new deprivation period

Not a Successfully Completed Test Sequence

EXHIBIT G-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
STANDARD QUALITY ASSURANCE PROCEDURES
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST D. Ashby #5162 AGENCY Y080
DATE 12-24-08 TIME 0755
INTOXILYZER SERIAL # 800001456 LOCATION Yarnell Substation

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution 1.00 AC.
OR
Pour a standard alcohol concentration solution _____ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 097 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

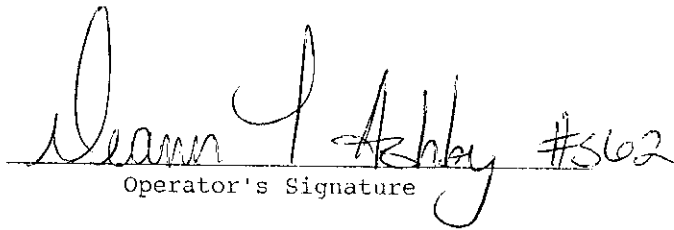
SIGNATURE D. Ashby #5162 DAS# 33400

INTOXILYZER 8000
Location: YAVAPAI SO YARNELL
Serial Number: 80-001456
12/24/2008 07:55:33

Standard Lot#: 7309011
Last Changed By: C. KROGEDAL #6535

QAS: D. ASHBY #S62
YAVAPAI CSO

Test	g/210L	Time
Air Blank	0.000	07:56:01
Cal Check	0.097	07:56:20
Air Blank	0.000	07:56:49


Operator's Signature #S62 QAS#33400