

EXHIBIT G-2  
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST D. Anderson #252 AGENCY Prescott PD  
DATE 052811 TIME 1959  
INTOXILYZER SERIAL # 80-000337 LOCATION PPD

- () 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution .100 AC.  
OR  
Pour a standard alcohol concentration solution \_\_\_\_\_ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- () 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- () 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- () 4. Air blank completed.
- () 5. Calibration check completed. Test results 0. 099 AC.
- () 6. Air blank completed.
- () 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE [Signature] #252

DPS Form Exh G-2 (Rev 05-01)

\* PRIOR TO GAS BOTTLE CHANGE.  
[Signature]

INTOXILYZER 8000

Location: PRESCOTT P.D

Serial Number: 80-000337

Core Version: 8105.48

05/28/2011

19:59:19

-----  
Standard Lot#: 25310100A1

Last Changed By: T. ATTENBERGER #252  
-----

QAS: T. ATTENBERGER #252

PRESCOTT PD  
-----

Operator: T. ATTENBERGER #252

PRESCOTT PD  
-----

Test	g/210L	Time
Air Blank	0.000	19:59:49
0.100 Cal Check	0.099	20:00:10
Air Blank	0.000	20:00:40

Preventative Maintenance

Performed -- Timer Reset

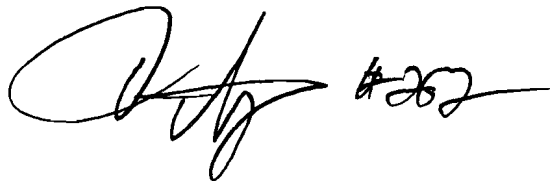


EXHIBIT G-2  
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000  
STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST T. Anderson #252 AGENCY Prescott P.D.  
DATE 052811 TIME 2007  
INTOXILYZER SERIAL # 8D-000337 LOCATION RPD.

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution. 100 AC.  
OR  
Pour a standard alcohol concentration solution                      AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach 34°C ± 0.2°C
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 097 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE [Signature]

DPS Form Exh G-2 (Rev 05-01)



G-2, G-4, G-2 AFTER BOTTLE CHANGE.

[Signature]

INTOXILYZER 8000

Location: PRESCOTT P.D

Serial Number: 80-000337

Core Version: 8105.48

05/28/2011

20:07:19

-----  
Standard Lot#: 25310100A1

Last Changed By: T. ATTENBERGER #252

-----  
QAS: T. ATTENBERGER #252

PRESCOTT PD

-----  
Operator: T. ATTENBERGER #252

PRESCOTT PD

-----  
Test                      g/210L                      Time  
-----  
Air Blank                      0.000                      20:07:50  
0.100 Cal Check                      0.097                      20:08:11  
Air Blank                      0.000                      20:08:41

Preventative Maintenance  
Performed -- Timer Reset

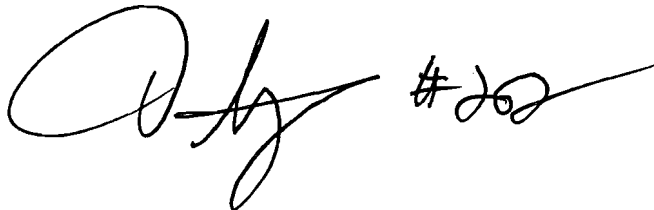
A handwritten signature in black ink, consisting of a large, stylized initial 'T' followed by the number '#252' and a long horizontal flourish.

EXHIBIT G-4  
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST T. Amberg #252 AGENCY Phoenix P.D.  
DATE 0528/11 TIME 2011  
INTOXILYZER SERIAL # 80-000337 LOCATION P.P.D.

1. Display Reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

1. Clock time check.  
 2. Date check.

OPERATIONAL TESTS

1. Alcohol-free subject test result 0. 000 AC.  
 2. Error recognition logic system functioning.  
Not a Successfully Completed Test Sequence printed  
 3. Proper sample recognition system.  
Not a Successfully Completed Test Sequence printed  
Deficient sample printed.  
 4. Standard Calibration Check standard 0. 100 AC. Result 0. 097 AC.

Instrument is operating properly and accurately. YES  NO

COMMENTS

ALL FUNCTIONING CORRECTLY.

SIGNATURE [Signature] #252

INTOXILYZER 8000  
Location: PRESCOTT P.D  
Serial Number: 80-000337  
Core Version: 8105.48  
05/28/2011 20:11:17

---

Standard Lot#: 25310100A1  
Last Changed By: T. ATTENBERGER #252

---

QAS: T. ATTENBERGER #252  
PRESCOTT PD

---

Operator: T. ATTENBERGER #252  
PRESCOTT PD

---

Subject: SQAP, TEST  
DOB: 01/01/1900  
Sex: M Weight: 300


---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	20:12:21
Diagnostic Test	Pass	20:12:55
Air Blank	0.000	20:13:22
0.100 Cal Check	0.097	20:13:43
Air Blank	0.000	20:14:12
Subject Test	0.000	20:14:34
Air Blank	0.000	20:15:01
Wait	ABT*	
Air Blank	0.000	20:15:39

\*Sequence Aborted

A handwritten signature in black ink, appearing to be "T. Attenberger", written in a cursive style.

**Not a Successfully Completed Test Sequence**

INTOXILYZER 8000  
Location: PRESCOTT P.D  
Serial Number: 80-000337  
Core Version: 8105.48  
05/28/2011 20:16:10

---

Standard Lot#: 25310100A1  
Last Changed By: T. ATTENBERGER #252

---

QAS: T. ATTENBERGER #252  
PRESCOTT PD

---

Operator: T. ATTENBERGER #252  
PRESCOTT PD

---

Subject: SQAP, TEST  
DOB: 01/01/1900  
Sex: M Weight: 300

---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	IPS*	20:16:48
Air Blank	0.000	20:17:16

\*Improper Sample



**Not a Successfully Completed Test Sequence**

INTOXILYZER 8000

Location: PRESCOTT P.D

Serial Number: 80-000337

Core Version: 8105.48

05/28/2011

20:17:55

---

Standard Lot#: 25310100A1

Last Changed By: T. ATTENBERGER #252

---

QAS: T. ATTENBERGER #252

PRESCOTT PD

---

Operator: T. ATTENBERGER #252

PRESCOTT PD

---

Subject: SQAP, TEST

DOB: 01/01/1900

Sex: M

Weight: 300


---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	RFI*	20:18:39
Air Blank	0.000	20:19:08

\*RFI Detect

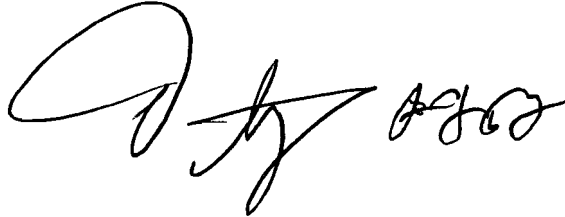A handwritten signature in black ink, appearing to be 'T. Attenberger', is written over the text '\*RFI Detect'.

**Not a Successfully Completed Test Sequence**

INTOXILYZER 8000  
Location: PRESCOTT P.D  
Serial Number: 80-000337  
Core Version: 8105.48  
05/28/2011 20:19:40

---

Standard Lot#: 25310100A1  
Last Changed By: T. ATTENBERGER #252

---

QAS: T. ATTENBERGER #252  
PRESCOTT PD

---

Operator: T. ATTENBERGER #252  
PRESCOTT PD

---

Subject: SQAP, TEST  
DOB: 01/01/1900  
Sex: M Weight: 300

---

15 Minute Deprivation Period? Yes


---

Test	g/210L	Time
Air Blank	0.000	20:20:
Diagnostic Test	Pass	20:21:
Air Blank	0.000	20:21:
0.100 Cal Check	0.097	20:21:
Air Blank	0.000	20:22:
Subject Test	0.023*	20:25:
Air Blank	0.000	20:26:
Air Blank	0.000	20:26:
Subject Test	XXX**	20:27:
Air Blank	0.000	20:27:

\*Deficient Sample

\*\*Invalid Sample

Begin new deprivation period

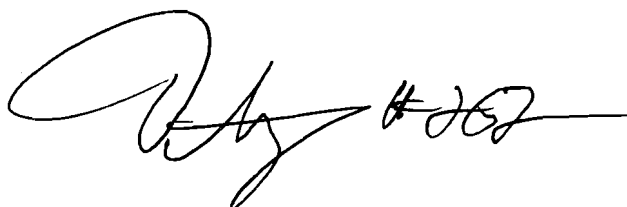A handwritten signature in black ink, appearing to be 'T. Attenberger', with a horizontal line extending to the right.

Not a Successfully Completed Test Se

EXHIBIT G-2  
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST T. H. [Signature] #252 AGENCY Reynolds P.D.  
DATE 052811 TIME 2028  
INTOXILYZER SERIAL # 88-000337 LOCATION R.P.D.

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution. 100 AC.  
OR  
Pour a standard alcohol concentration solution AC into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach  $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 097 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE [Signature]

INTOXILYZER 8000

Location: PRESCOTT P.D

Serial Number: 80-000337

Core Version: 8105.48

05/28/2011

20:28:19

-----  
Standard Lot#: 25310100A1

Last Changed By: T. ATTENBERGER #252  
-----

QAS: T. ATTENBERGER #252

PRESCOTT PD  
-----


Operator: T. ATTENBERGER #252

PRESCOTT PD  
-----

Test	g/210L	Time
Air Blank	0.000	20:28:50
0.100 Cal Check	0.097	20:29:11
Air Blank	0.000	20:29:40

Preventative Maintenance

Performed -- Timer Reset

A handwritten signature in black ink, consisting of a large, stylized initial 'T' followed by a smaller, less distinct signature.