

EXHIBIT G-2  
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST D. Agnew #252 AGENCY Prescott P.D.  
DATE 08/23/12 TIME 1004  
INTOXILYZER SERIAL # 80-000337 LOCATION P.P.D.

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution -100 AC.  
OR  
Pour a standard alcohol concentration solution \_\_\_\_\_ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach  $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select D for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0.097 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE [Signature] #252

DPS Form Exh G-2 (Rev 05-01)

MC

INTOXILYZER 8000

Location: PRESCOTT P.D

Serial Number: 80-000337

Core Version: 8105.48

08/23/2012

10:04:08

-----  
Standard Lot#: 09312100A1

Last Changed By: T. ATTENBERGER #252

-----  
QAS: T. ATTENBERGER #252

PRESCOTT PD

-----  
Operator: T. ATTENBERGER #252

PRESCOTT PD

-----  
Test                      g/210L                      Time  
-----  
Air Blank                      0.000                      10:04:39  
0.100 Cal Check                0.097                      10:05:00  
Air Blank                      0.000                      10:05:29

Preventative Maintenance  
Performed -- Timer Reset

 #252

EXHIBIT G-4  
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000

STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST T. Anderson DSP 602 #052 AGENCY Prescott P.D.  
DATE 08/23/12 TIME 1006  
INTOXILYZER SERIAL # 80-000337 LOCATION P.P.D.

1. Display Reads "PUSH BUTTON TO START"

DIAGNOSTIC TESTS

1. Clock time check.  
 2. Date check.

OPERATIONAL TESTS

1. Alcohol-free subject test result 0. 000 AC.  
 2. Error recognition logic system functioning.  
Not a Successfully Completed Test Sequence printed  
 3. Proper sample recognition system.  
Not a Successfully Completed Test Sequence printed  
Deficient sample printed.  
 4. Standard Calibration Check standard 0. 100 AC. Result 0. 096 AC.

Instrument is operating properly and accurately. YES  NO

COMMENTS

ALL FUNCTIONING CORRECTLY.

SIGNATURE T. Anderson #052

INTOXILYZER 8000

Location: PRESCOTT P.D

Serial Number: 80-000337

Core Version: 8105.48

08/23/2012

10:06:39

---

Standard Lot#: 09312100A1

Last Changed By: T. ATTENBERGER #252

---

QAS: T. ATTENBERGER #252  
PRESCOTT PD

---

Operator: T. ATTENBERGER #252  
PRESCOTT PD

---

Subject: SQAP, TEST

DOB: 01/01/1900

Sex: M Weight: 300

---


15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	0.000	10:07:49
Diagnostic Test	Pass	10:08:23
Air Blank	0.000	10:08:51
0.100 Cal Check	0.097	10:09:11
Air Blank	0.000	10:09:41
Subject Test	0.000	10:09:57
Air Blank	0.000	10:10:25
Wait	ABT*	
Air Blank	0.000	10:11:00

---

\*Sequence Aborted

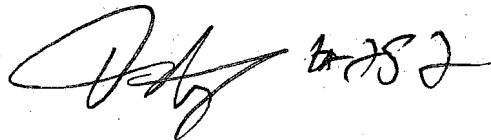

Not a Successfully Completed Test Sequence

INTOXILYZER 8000

Location: PRESCOTT P.D

Serial Number: 80-000337

Core Version: 8105.48

08/23/2012

10:11:36

---

Standard Lot#: 09312100A1

Last Changed By: T. ATTENBERGER #252

---

QAS: T. ATTENBERGER #252  
PRESCOTT PD

---

Operator: T. ATTENBERGER #252  
PRESCOTT PD

---

Subject: SQAP, TEST

DOB: 01/01/1900

Sex: M

Weight: 300


---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	IPS*	10:12:15
Air Blank	0.000	10:12:43

\*Improper Sample

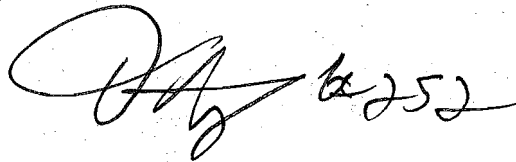

A handwritten signature in black ink, appearing to read 'T. Attenberger #252', is written over the printed text.

---

**Not a Successfully Completed Test Sequence**

INTOXILYZER 8000

Location: PRESCOTT P.D

Serial Number: 80-000337

Core Version: 8105.48

08/23/2012

10:13:08

---

Standard Lot#: 09312100A1

Last Changed By: T. ATTENBERGER #252

---

QAS: T. ATTENBERGER #252  
PRESCOTT PD

---

Operator: T. ATTENBERGER #252  
PRESCOTT PD

---

Subject: SQAP, TEST

DOB: 01/01/1900

Sex: M

Weight: 300


---

15 Minute Deprivation Period? Yes

---

Test	g/210L	Time
Air Blank	RFI*	10:13:43
Air Blank	0.000	10:14:12

\*RFI Detect

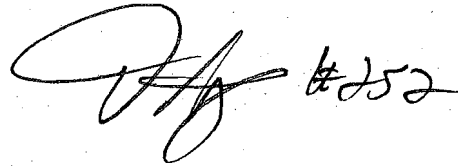 #252

---

Not a Successfully Completed Test Sequence

INTOXILYZER 8000  
Location: PRESCOTT P.D  
Serial Number: 80-000337  
Core Version: 8105.48  
08/23/2012

10:14:41

---

Standard Lot#: 09312100A1  
Last Changed By: T. ATTENBERGER #252

---

QAS: T. ATTENBERGER #252  
PRESCOTT PD

---

Operator: T. ATTENBERGER #252  
PRESCOTT PD

---

Subject: SQAP, TEST  
DOB: 01/01/1900  
Sex: M Weight: 300

---

15 Minute Deprivation Period? Yes

---


Test	g/210L	Time
Air Blank	0.000	10:15:31
Diagnostic Test	Pass	10:16:05
Air Blank	0.000	10:16:32
0.100 Cal Check	0.096	10:16:53
Air Blank	0.000	10:17:23
Subject Test	0.046*	10:20:30
Air Blank	0.000	10:21:02
Air Blank	0.000	10:21:29
Subject Test	XXX**	10:22:09
Air Blank	0.000	10:22:42

---

\*Deficient Sample

\*\*Invalid Sample

Begin new deprivation period

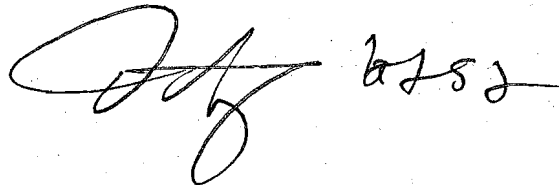

Not a Successfully Completed Test Sequence

EXHIBIT G-2  
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY  
STANDARD QUALITY ASSURANCE PROCEDURES  
INTOXILYZER MODEL 8000  
STANDARD CALIBRATION CHECK PROCEDURE

QA SPECIALIST T. ADENBARGER #252 AGENCY Prescott P.D.  
DATE 08/23/12 TIME 1023  
INTOXILYZER SERIAL # 80-000337 LOCATION P.P.D.

- (✓) 1. Ensure that gas tank is attached to instrument and contains a standard alcohol concentration solution .100 AC.  
OR  
Pour a standard alcohol concentration solution \_\_\_\_\_ AC, into a clean dry simulator and assemble the simulator. Ensure that a tight seal has been made. Turn on the simulator and allow temperature to reach  $34^{\circ}\text{C} \pm 0.2^{\circ}\text{C}$
- (✓) 2. Intoxilyzer 8000 display reads "PUSH BUTTON TO START"
- (✓) 3. Go to the "Control Testing Menu". Select "D" for dry control test or "W" for wet control test. After selection is made press ENTER.
- (✓) 4. Air blank completed.
- (✓) 5. Calibration check completed. Test results 0. 096 AC.
- (✓) 6. Air blank completed.
- (✓) 7. Remove printed record. Attach the record to the completed checklist.

SIGNATURE [Signature] #252

INTOXILYZER 8000  
Location: PRESCOTT P.D  
Serial Number: 80-000337  
Core Version: 8105.48  
08/23/2012

10:23:47


-----  
Standard Lot#: 09312100A1  
Last Changed By: T. ATTENBERGER #252  
-----

QAS: T. ATTENBERGER #252  
PRESCOTT PD  
-----

Operator: T. ATTENBERGER #252  
PRESCOTT PD  
-----

Test	g/210L	Time
Air Blank	0.000	10:24:16
0.100 Cal Check	0.096	10:24:37
Air Blank	0.000	10:25:07

Preventative Maintenance  
Performed -- Timer Reset

 #252