

EXHIBIT I-2

THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
INTOXILYZER MODEL 9000

PERIODIC MAINTENANCE AND STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST N. Namenny AGENCY Prescott Police Department
DATE 3/20/2026 TIME 2244
INTOXILYZER SERIAL # 9U-005776

☒ 1. Ensure that gas tank is attached and contains a standard alcohol concentration 2.10 AC

DIAGNOSTIC TESTS

- ☒ 1. Clock time check
☒ 2. Date check

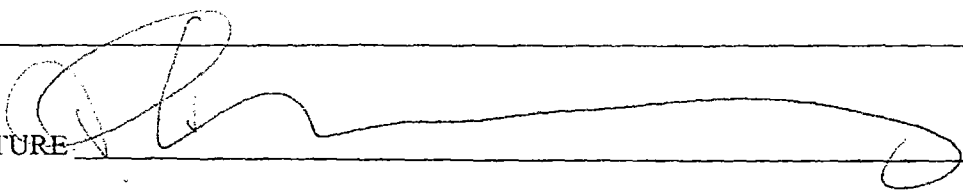
OPERATIONAL TESTS

- ☒ 1. Deficient Subject Test (Proper Sample Recognition)
Deficient Sample printed
☒ 2. Alcohol-free Subject Test (Proper Sample Recognition):
0.800 AC
☒ 3. Mouth Alcohol Subject Test (Proper Sample Recognition):
Invalid Sample – Begin new deprivation period printed
☒ 4. Radio Frequency Interference Test (Error Recognition):
RFI Detect printed
☒ 5. Standard Calibration Check:
0.299 AC
☒ 6. Air Blanks Completed
☒ 7. Timer Reset

Not a Successfully Completed Test Sequence will be printed

Instrument is operating properly and accurately. YES ☒ NO ☐

COMMENTS:

SIGNATURE 

ARIZONA FORENSIC BREATH ALCOHOL ANALYTICAL REPORT

INSTRUMENT INFORMATION

Analytical Instrument: Intoxilyzer 9000
Serial Number: 90-005776
Software Version: 9439.01.00
Analytical Report Number: 57760320260197

QAS: REED, PERRY
QAS Permit #: 30248
Agency: PRESCOTT PD
Last 31-Day Check: 01/01/2026
Last Annual Maintenance: 01/08/2026

SUBJECT INFORMATION

Name: 31-Day Check
Test Date: 03/20/2026
Driver's License #:
Gender:
Date of Birth:
Age:

Weight:
State of Issue:
Driver's License Expiration:
Deprivation Start Time: 22:45
15 - Minute Deprivation: Yes

OPERATOR INFORMATION

Name: NAMANNY, NATHANIEL
Agency: AZ DPS

Permit #: 30250
STANDARD INFORMATION
Standard Value: 0.100
Standard Lot #: 15924100A1
Expiration Date: 07/05/2026
Bottle #: 5
Last Changed By: NAMANNY, NATHANIEL

Permit #: 30250

Test	g/210L	Time
Air Blank	0.000	23:03:24
Diagnostic Test	PASS	23:04:00
Air Blank	0.000	23:04:36
Calibration Chk	0.099	23:04:58
Air Blank	0.000	23:05:38
Subject Test 1	DEF*	23:09:22
Air Blank	0.000	23:10:14
Air Blank	0.000	23:10:55
Subject Test 2	0.000	23:11:25
Air Blank	0.000	23:12:10
Wait		23:16:14
Air Blank	0.000	23:16:51
Subject Test 3	INV**	23:19:56
Air Blank	RFI***	23:20:09

RESULTS

EXCEPTION MESSAGES

*Deficient Sample
**Invalid Sample - Begin new deprivation period
***RFI Detect

* Deficient Sample
** Invalid Sample - Begin new deprivation period
*** RFI Detect

OPERATOR COMMENTS

Not a Successfully Completed Test Sequence

*All air blank results must be 0.000.
Consecutive subject test results must not differ by more than 0.020 g/210L.
Standard check results must be $\pm 10\%$.*

Intoxilyzer - Alcohol Analyzer

Model 9000

SN: 90-005776

Test Date: 03/20/2026

Test Time: 23:25

Location:

Software Version: 9439.01.00

Standard Lot #: 15924100A1

Standard Value: 0.100

Expiration Date: 07/05/2026

Bottle #: 5

Last Changed By: NAMANNY, NATHANIEL

Permit #: 30250

Operator: NAMANNY, NATHANIEL

Permit #: 30250

Agency: AZ DPS

Test	g/210L	Time
Air Blank	0.000	23:25:34
Calibration Chk	0.099	23:25:56
Air Blank	0.000	23:26:35

No RFI Detected