

EXHIBIT I-2
THIS REPORT PREPARED PURSUANT TO DUTY IMPOSED BY A.A.C. R13-10-104 (A)

ARIZONA DEPARTMENT OF PUBLIC SAFETY
INTOXILYZER MODEL 9000

PERIODIC MAINTENANCE AND STANDARD QUALITY ASSURANCE PROCEDURE

QA SPECIALIST N. Nemony AGENCY Prescott PD
DATE 5/21/2026 TIME 1819
INTOXILYZER SERIAL # 50-005776

☒ 1. Ensure that gas tank is attached and contains a standard alcohol concentration .10 AC

DIAGNOSTIC TESTS

- ☒ 1. Clock time check
☒ 2. Date check

OPERATIONAL TESTS

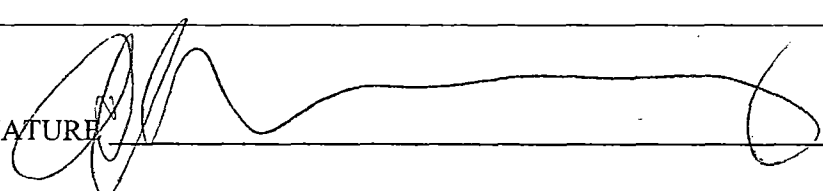
- ☒ 1. Deficient Subject Test (Proper Sample Recognition)
Deficient Sample printed
- ☒ 2. Alcohol-free Subject Test (Proper Sample Recognition):
0.000 AC
- ☒ 3. Mouth Alcohol Subject Test (Proper Sample Recognition):
Invalid Sample – Begin new deprivation period printed
- ☒ 4. Radio Frequency Interference Test (Error Recognition):
RFI Detect printed
- ☒ 5. Standard Calibration Check:
0.100 AC
- ☒ 6. Air Blanks Completed
- ☒ 7. Timer Reset

Not a Successfully Completed Test Sequence will be printed

Instrument is operating properly and accurately. YES ☒ NO ☐

COMMENTS:

- Had to do Invalid Sample. Exceeded limit.

SIGNATURE 

ARIZONA FORENSIC BREATH ALCOHOL ANALYTICAL REPORT

INSTRUMENT INFORMATION

Analytical Instrument: Intoxilyzer 9000
Serial Number: 90-005776
Software Version: 9439.01.00
Analytical Report Number: 57760521260256

QAS: NAMANNY, NATHANIEL
QAS Permit #: 30250
Agency: AZ DPS
Last 31-Day Check: 04/20/2026
Last Annual Maintenance: 01/08/2026

SUBJECT INFORMATION

Name: 31-Day Check
Test Date: 05/21/2026
Driver's License #:
Gender:
Date of Birth:
Age:

Weight:
State of Issue:
Driver's License Expiration:
Deprivation Start Time: 18:00
15 - Minute Deprivation: Yes

OPERATOR INFORMATION

Name: NAMANNY, NATHANIEL
Agency: AZ DPS

Permit #: 30250

STANDARD INFORMATION

Standard Value: 0.100
Standard Lot #: 30325100A3
Expiration Date: 07/05/2026
Bottle #: 6
Last Changed By: NAMANNY, NATHANIEL

Permit #: 30250

Test	g/210L	Time
Air Blank	0.000	18:21:33
Diagnostic Test	PASS	18:22:09
Air Blank	0.000	18:22:46
Calibration Chk	0.099	18:23:08
Air Blank	0.000	18:23:47
Subject Test 1	DEF*	18:27:05
Air Blank	0.000	18:27:57
Air Blank	0.000	18:28:37
Subject Test 2	0.000	18:29:47
Air Blank	0.000	18:30:29
Wait		18:34:34
Air Blank	0.000	18:35:11
Subject Test 3	RNG**	18:36:07
Air Blank	RFI***	18:36:20

*Deficient Sample
**Range Exceeded
***RFI Detect

RESULTS

EXCEPTION MESSAGES

* Deficient Sample
** Range Exceeded
*** RFI Detect

OPERATOR COMMENTS

Not a Successfully Completed Test Sequence

*All air blank results must be 0.000.
Consecutive subject test results must not differ by more than 0.020 g/210L.
Standard check results must be $\pm 10\%$.*

ARIZONA FORENSIC BREATH ALCOHOL ANALYTICAL REPORT

INSTRUMENT INFORMATION

Analytical Instrument: Intoxilyzer 9000
Serial Number: 90-005776
Software Version: 9439.01.00
Analytical Report Number: 57760521260257

QAS: NAMANNY, NATHANIEL
QAS Permit #: 30250
Agency: AZ DPS
Last 31-Day Check: 05/21/2026
Last Annual Maintenance: 01/08/2026

SUBJECT INFORMATION

Name: 31-Day Check
Test Date: 05/21/2026
Driver's License #:
Gender:
Date of Birth:
Age:

Weight:
State of Issue:
Driver's License Expiration:
Deprivation Start Time: 18:00
15 - Minute Deprivation: Yes

OPERATOR INFORMATION

Name: NAMANNY, NATHANIEL
Agency: AZ DPS

Permit #: 30250

STANDARD INFORMATION

Standard Value: 0.100
Standard Lot #: 30325100A3
Expiration Date: 07/05/2026
Bottle #: 6
Last Changed By: NAMANNY, NATHANIEL

Permit #: 30250

Test	g/210L	Time
Air Blank	0.000	18:40:07
Diagnostic Test	PASS	18:40:44
Air Blank	0.000	18:41:21
Calibration Chk	0.098	18:41:42
Air Blank	0.000	18:42:22
Subject Test 1	INV*	18:42:38
Air Blank	RFI**	18:42:52

*Invalid Sample - Begin new deprivation period
**RFI Detect

RESULTS

EXCEPTION MESSAGES

* Invalid Sample - Begin new deprivation period
** RFI Detect

OPERATOR COMMENTS

Not a Successfully Completed Test Sequence

*All air blank results must be 0.000.
Consecutive subject test results must not differ by more than 0.020 g/210L.
Standard check results must be $\pm 10\%$.*

Intoxilyzer - Alcohol Analyzer
Model 9000

SN: 90-005776

Test Date: 05/21/2026

Test Time: 18:19

Location:

Software Version: 9439.01.00

Standard Lot #: 30325100A3

Standard Value: 0.100

Expiration Date: 07/05/2026

Bottle #: 6

Last Changed By: NAMANNY, NATHANIEL

Permit #: 30250

Operator: NAMANNY, NATHANIEL

Permit #: 30250

Agency: AZ DPS

Test	g/210L	Time
Air Blank	0.000	18:19:32
Calibration Chk	0.100	18:19:53
Air Blank	0.000	18:20:33

No RFI Detected